



EN

F-826
Instruction Manual
WE-2013-F826-1

PRESSOTHERAPY

WARNING


- Never under any circumstances attempt to open or inspect the internal components or accessories of the machine. If an inspection becomes necessary, please contact your supplier or a suitably competent technician.
- Never use the unit in humid or poorly ventilated environments, such as wet rooms, bathrooms, etc. to prevent damage to the electrical components of your unit.
- Never use the unit outdoors; exposure to the elements can cause damage.
- If the power cord was destroyed, please ask a professional to service and replace it to avoid hazards, or contact the dealer for service.

EC-DECLARATION OF COMPLIANCE

This product meets the following requirements:

1. Conditions set out in the Low Voltage Directive: 2006/95/EC
2. Conditions set out in the Electromagnetic Compatibility Directive: 2004/108/EC

RECYCLING

 Whenever any of our electrical products or their presentation packaging bear this symbol, it means that these products should not be treated as conventional household waste in Europe. To ensure proper treatment of this waste, dispose of it in accordance with local laws or as required for the disposal of electrical equipment. This initiative will help preserve save natural resources and improve standards of environmental protection in regard to the treatment of electrical waste.

WELCOME!

Thank you very much for purchase. Please read the instructions carefully before operating the instrument. You can also ask a professional for guidance to make sure you are using the instrument correctly. We will accept no responsibility for any accidents that occur due to

incorrect operation.



The company reserves the right to amend the details of the instruments with no prior notice. If any mistakes are found in these instructions, please feel free to send us an e-mail informing us so that we can correct them.

PACKAGE CONTENTS

- These components are subject to change without prior notice.
- Appearance of product may differ from the image.

| No. | PRODUCT | REF. | QTY. |
|-----|--------------|---------------|------|
| 1 | RIGHT BOOT | 40001-1 40001 | 1 |
| 2 | LEFT BOOT | 40001-2 | 1 |
| 3 | RIGHT ARM | 40001-3 | 1 |
| 4 | LEFT ARM | 40001-4 | 1 |
| 5 | WAIST | 40001-5 | 1 |
| 6 | TUBES | 40001-6 | 1 |
| 7 | MAIN UNIT | - | 1 |
| 8 | FEEDER CABLE | - | 1 |





FRONT PANEL/REAR PANEL

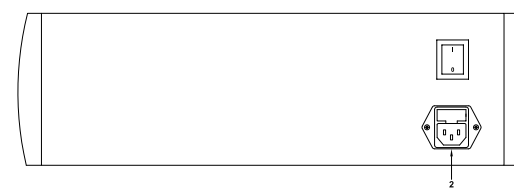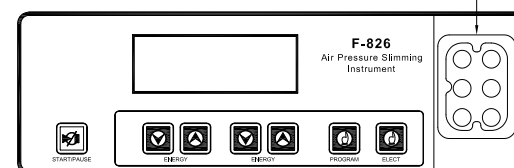


1. Pressotherapy tubes
2. Power line input

INSTRUCTIONS OF USE

1. Connect the power supply via the rear panel, indicated in the sketch as "POWER LINE INPUT".
2. Separate the ends of the tubes with scissors. Never try to pull them apart with your hands.

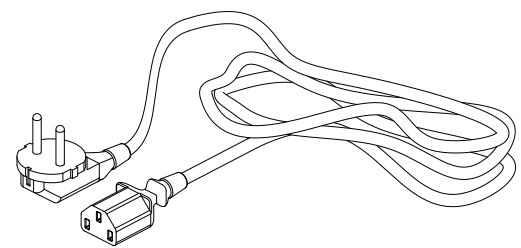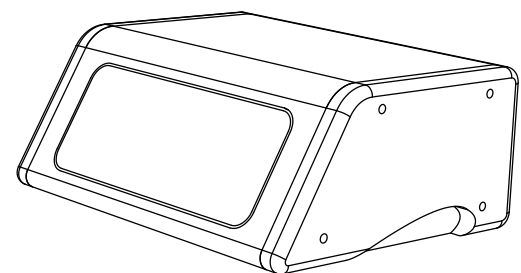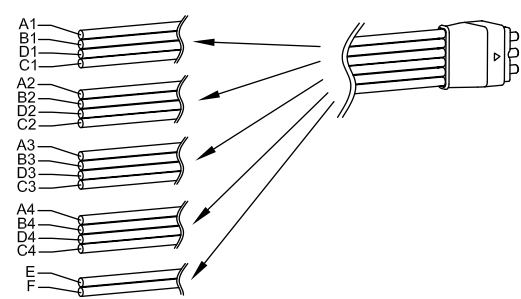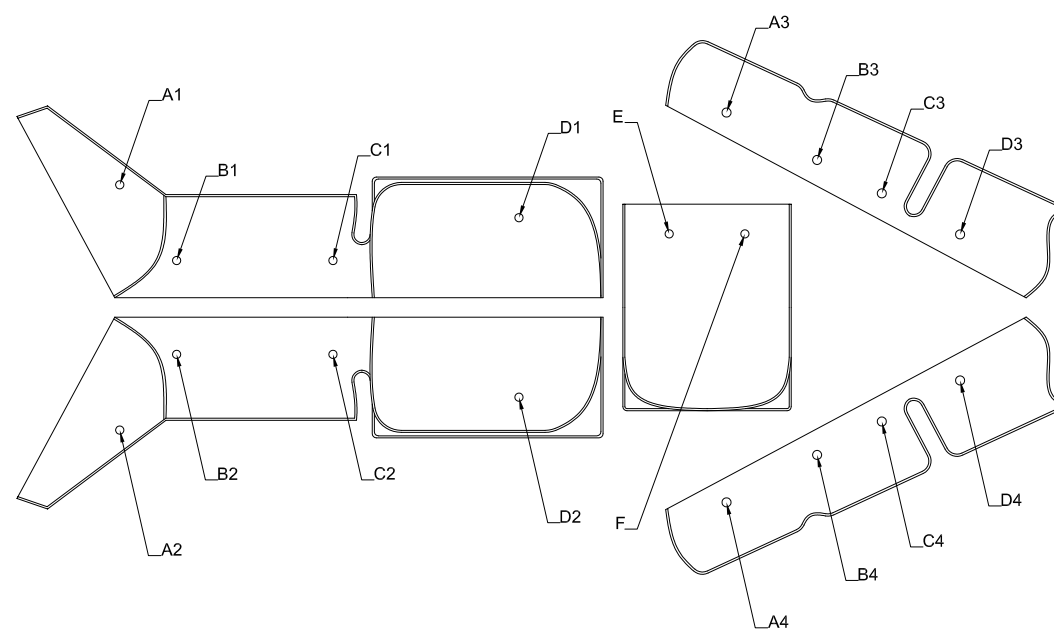

3. Connect the accessories properly to the front/rear panel as indicated in the sketch.
4. Connect all tubes to the main frame and airbags as indicated in the sketch.

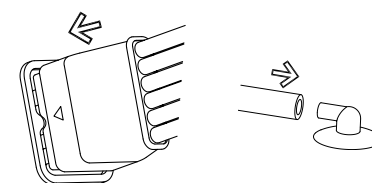

5. Wrap the airbag around the user's body.
6. Turn on the "POWER BUTTON" on the rear panel. At this moment, the screen displays "PROGRAM: A", "TIMER: 15", "ENERGY: 04" and "FULLBODY".
7. Select the required time and air pressure. The maximum "TIMER" value is "60" minutes and the maximum "ENERGY" value is "10".
8. Select the desired mode by pressing "PROGRAM". Three modes are available: A, B, C.

- Mode A: Each section is filled with air in 8 seconds and the air is then vented, circulating twice. Later, each section is filled with air in sequence within 8 seconds and filled continuously, and then the air is vented in 5 seconds at the same time. This

is a whole cycle.

- Mode B: Each section is filled with air in sequence within 3 seconds; then, for the last section, the air filling time is 5 seconds. Next, all the air is vented in 5 seconds. This is a whole cycle.

- Mode C: The air is filled separately in 10 seconds and then the air is vented in 3 seconds. This is a whole cycle.

9. Select the section by pressing the "SELECT" button. You can choose from the following three sections: abdomen, full body and hands & feet.

10. Press the "START/PAUSE" button to begin working. All the buttons can be adjusted when working.

CAUTIONS

- Be careful not to wrap the airbag too tight, to avoid hurting the users when the air is too strong.
- Check that all the tubes are properly connected.
- The air pressure should not be set too high to avoid causing pain.
- When the machine is working, a professional must be next to it controlling it.

ACCESSORIES

| REF. | DESCRIPTION |
|-------|--------------------|
| 40001 | 40001-1 RIGHT BOOT |
| | 40001-2 LEFT BOOT |
| | 40001-3 RIGHT ARM |
| | 40001-4 LEFT ARM |
| | 40001-5 WAIST |
| | 40001-6 TUBES |

TECHNICAL SHEET

| | | |
|----------------------------|---------------------|-------------|
| Weights and sizes | Packing size (cm) | 61x45x18,5 |
| | Gross weight (kg) | 13,5 |
| | Product size (cm) | 41x17/24x13 |
| Working characteristics | Working power | 75 W |
| | Working pressure | 0,32 bar |
| | Preset working time | 15 min |
| Electrical characteristics | Rated voltage | 220V ~ 240V |
| | Frequency | 50Hz/60Hz |
| | Rated power | 75 W |